



VPM18-13800

Description:

The toroidal construction inherently reduces stray fields, increases efficiency and minimizes size compared to traditional EI transformers. The addition of a Flux Band further reduces the remaining stray fields. The shield between Primary and Secondary improves safety, reduces common mode signals and minimizes leakage current. Built with a Class F (155°) insulation system. A 140°C self-resetting thermal switch is included in each primary.

Electrical Specifications (@25C)

1. Maximum Power: 250VA
2. Input Voltages: 100, 120, 220, 240VAC, 50/60Hz
3. Output Voltages: 9VAC @27.60A or 18VAC CT @ 13.8A
4. Voltage Regulation: 6.2% TYP from full load to no load
5. Temperature Rise: 55°C TYP
6. Hipot: 4000VAC, Primary to Secondary, Primary & Secondary to Shield & mounting surface
7. Efficiency: 93% TYP. @ full load
8. Earth Leakage: $\leq 10\mu\text{A}$ (See Fig. 1), Patient Leakage: $\leq 25\mu\text{A}$ (see Fig. 2)

Agency File:

UL: File E122529, UL 60601-1/(R) 2012 Medical Electrical Equipment – Part 1 with 2 MOPP

CE: ES 60601-1 (IEC 60601-1:2005, MOD)

cUL: C22.2 No. 60601-1:14, Medical Electrical Equipment – Part 1

CB Certified.



Dimensions: Inches (mm)

O.D.	I.D.	HT.*
4.8 (123)	1.8(45)	2.4(60)

*Add 0.188 (3) to the height for mounting hardware

Weight: 2.5Kg

Mounting:

Transformer is provided with one metal mounting plate, two rubber pads, M6 x 65mm bolt, nut, spring and flat washer.

Connections:

Transformer is provided with 8" (203mm) long, 0.25" (6.35mm) stripped and tinned, stranded UL 1015 lead wire. Primaries are 20AWG, Secondaries are 12AWG, and Shield is 20AWG.

The GRN/YEL shield lead is typically grounded. Do not lift transformer by leads!

Input Options:

- 100VAC: Input to Gray & Blue, jumper White & Brown, jumper Blue & Violet.
- 120VAC: Input to White & Blue, jumper White & Brown, jumper Blue & Violet.
- 220VAC: Input to Gray & Violet, jumper Blue & Brown
- 240VAC: Input to White and Violet, jumper Blue & Brown




Output Options:

- 9VAC: Output from Black & Red, jumper Black & Orange, jumper Red to Yellow
- 18VAC: Output from Black & Yellow, jumper Red & Orange

Primary and secondary windings are designed to be connected in series or parallel. Windings are not intended to be used independently.

RoHS Compliance: Meets the requirements of 2011/65/EU, known as the RoHS 2 initiative.

* At printing, this document is considered "uncontrolled". Contact Triad Magnetics' website for current version

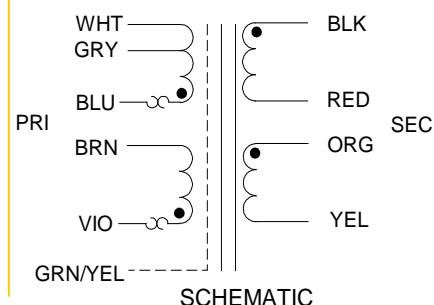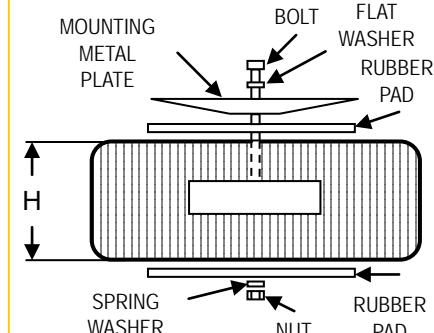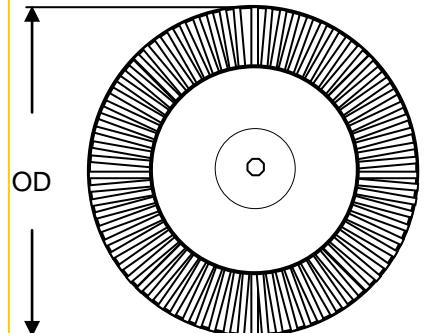



Earth Leakage Current:

V_{in} : Apply 264VAC @60Hz, BLU & BRN - YEL/GRN

Connect resistor and meter between: RED & ORG - YEL/GRN

$$\text{Leakage Current} = 10 \text{ uA MAX}$$

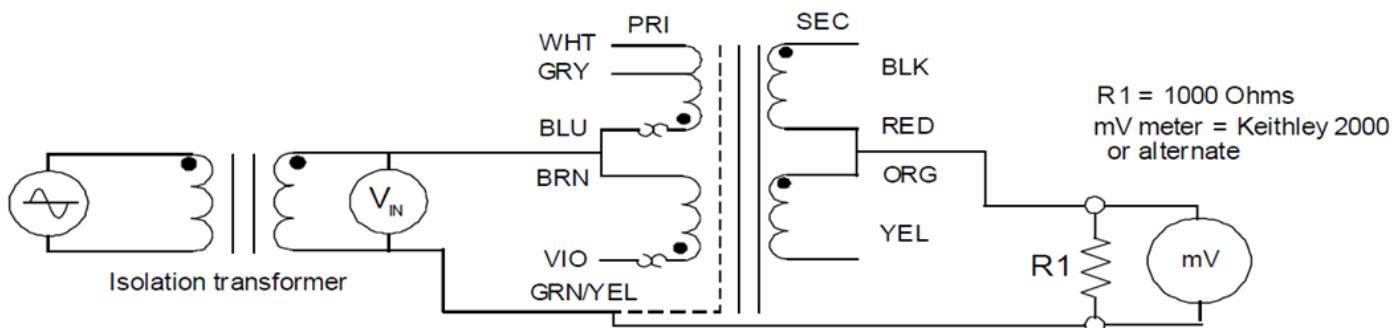


Figure 1

Patient Leakage Current:

V_{in} : Apply 264VAC @60Hz, WHT - VIO,

(Tie BLU & BRN, Tie RED & ORG)

$$\text{GRN/YEL - BLK} = 25 \text{ uARMS MAX}$$

$$\text{GRN/YEL - Red & ORG} = 25 \text{ uARMS MAX}$$

$$\text{GRN/YEL - YEL} = 25 \text{ uARMS MAX}$$

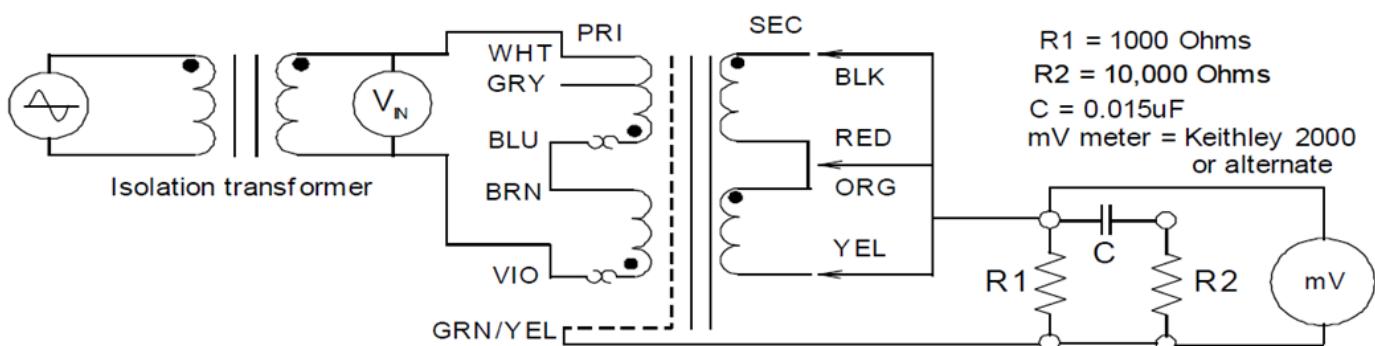


Figure 2