




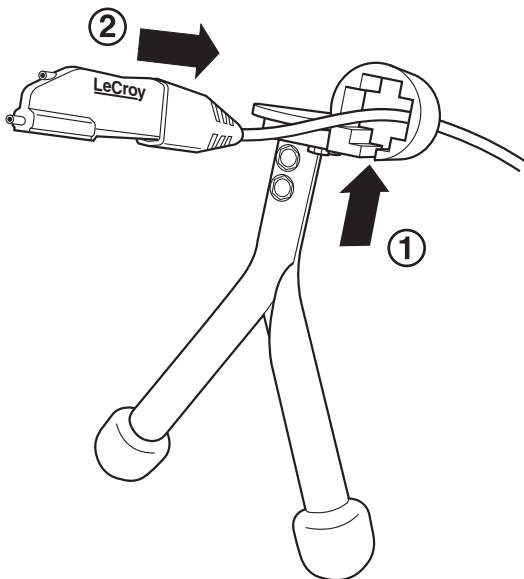


HFP Series Accessory Guide

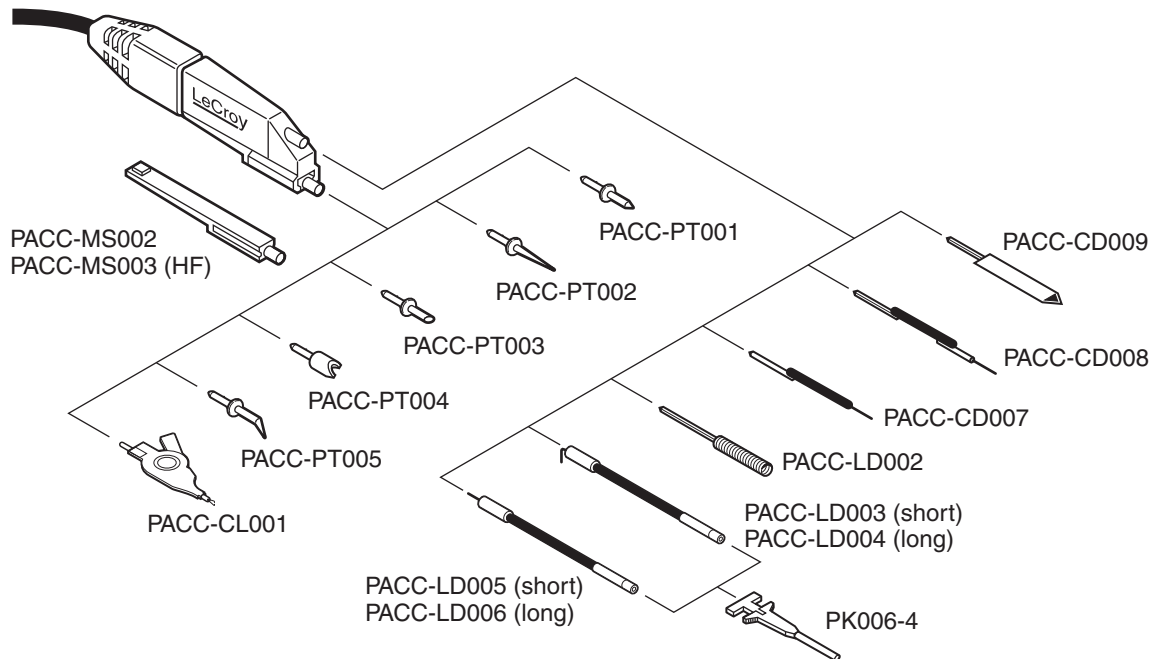

Installing the probe
into the FreeHand holder

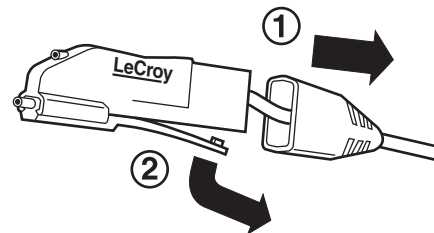

Removing the replaceable cartridge

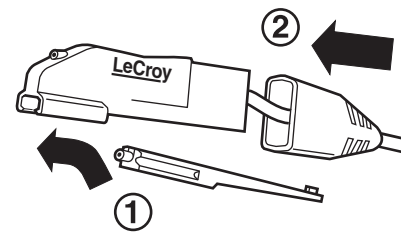

Installing a new cartridge

