

ADS62PXX EVM

User's Guide



Literature Number: SLAU237
May 2008

1	Overview.....	5
1.1	ADS62PXX EVM Quick-Start Procedure	5
2	Circuit Description	6
2.1	Schematic Diagram	6
2.2	ADC Circuit Function	6
3	TI ADC SPI Control Interface	9
3.1	Installing the ADC SPI Control Software	9
3.2	Setting Up the EVM for ADC SPI Control	10
3.3	Using the TI ADC SPI Interface Software	10
4	Connecting to FPGA Platforms	14
4.1	TSW1200	14
4.2	TSW1100	14
5	ADC Evaluation	15
5.1	Hardware Selection	15
5.2	Coherent Input Frequency Selection.....	16
6	Physical Description	17
6.1	PCB Layout.....	17
6.2	Bill of Materials.....	20
6.3	EVM Schematics	22
	Important Notices	28

List of Figures

1	Found New Hardware	9
2	Window Logo Testing.....	10
3	Hardware Device Manager.....	10
4	SPI Interface Screen	11
5	Top Silkscreen	17
6	Component Side.....	18
7	Power Plane 1	18
8	Bottom Side	19
9	EVM Schematic, Sheet 1.....	22
10	EVM Schematic, Sheet 2.....	23
11	EVM Schematic, Sheet 3.....	24
12	EVM Schematic, Sheet 4.....	25
13	EVM Schematic, Sheet 5.....	26
14	Breakout Board Schematic, Sheet 6.....	27

List of Tables

1	Jumpers	8
2	Surface-Mount Jumpers	8
3	ADS62PXX Frequently Used Registers	13
4	Bill of Materials	20

ADS62PXX EVM

1 Overview

This user's guide gives a general overview of the evaluation module (EVM) and provides a general description of the features and functions to be considered while using this module. This manual is applicable to the ADS62P42/43/44/45, ADS62P22/23/24/25 and ADS62P15/C15 analog to digital converters (ADC), which will be collectively referred to as ADS62PXX. This document should be used in combination with respective ADC data sheet.

This document should be used in combination with the respective ADC data sheet.

1.1 ADS62PXX EVM Quick-Start Procedure

Using the quick-start procedure, many users can begin evaluating the ADC in a short time. The quick-start uses the default conditions on the EVM as shipped from the factory. If users modify the default jumper settings, this procedure does not apply.

1. The EVM contains a linear power supply solution to provide the necessary voltage rails to the ADC and associated circuits. Simply connect +5 V to P5 and GND to P4. Short P4 and P2 together.
2. Connector J4 (SMA) is connected to the path of the ADC clock input. It is used to connect the ADC clock input with off-board clock source. A low phase-noise sine-wave clock source is recommended for default EVM setting.
3. Connectors J6 (SMA) and J3 (SMA) are used to connect ADC channel A and channel B, respectively with an off-board analog continuous-wave (CW) signal source.
4. Connect the TSW1200 or suitable logic analyzer to J8 to capture the resulting digital data (DDR LVDS format).

2 Circuit Description

2.1 Schematic Diagram

The schematic diagram for the EVM is in [Section 6.3](#).

2.2 ADC Circuit Function

The following sections describe the function of individual circuits. See the relevant data sheet for device operating characteristics.

2.2.1 ADC Operational Mode

By default, the ADC is configured to operate in parallel-mode operation, since jumper (JP11) asserts a 3.3-V state to the ADC reset pin. Consequently, the SW1 reset pushbutton must be pressed only when the device is configured in serial operation mode. Because the ADC is in parallel operation mode, voltages are used to set the ADC configuration modes. Users can use the EVM silkscreen to set the operation modes.

2.2.2 EVM Power Connections

Banana jacks P1 to P6 on the EVM are used to connect the EVM to off-board DC power supplies. Users are given two primary options for connecting the ADC power supplies. By default, the ADC's AVDD and DVDD voltage rails are generated using TI's TPS79633 linear regulators. Their attributes of ultra-low noise and high PSRR make them ideal choices for high speed ADC power supply design. To measure ADC-device current consumption, we've provided a second DC power supply can be directly connected to the ADC. Users can use jumpers JP15 and JP16, detailed in Table 1, to switch between power supply options.

2.2.3 ADC Analog Inputs

By default, the EVM is configured to accept an AC-coupled single-ended input source from SMAs J6 and J3; these correspond to ADC inputs channel A and channel B, respectively. The input path converts the single-ended signal into a differential signal using a 1:1 transformer. The inputs to the ADC must be DC-biased, which is accomplished by using the ADC VCM output.

Using SMA input J3, users can evaluate the ADC using a [THS4509](#) amplifier, which converts a single-ended input into a differential signal while providing 10 dB of signal gain. The output path of the amplifier is AC coupled, and the DC is restored using the ADC VCM output. To use this evaluation path, please follow the steps below.

1. By default, the amplifier path is powered down. To turn on the THS4509, move the jumper found at JP3 to short positions 1-2.
2. Supply 5V DC to VS+ (P5) and connect ground to VS– (P6).
3. For AC-coupled evaluation setups, remove R72. This will force the amplifier common mode to Vss/2.
4. To connect the SMA input J3 to the amplifier inverting input terminal, short positions 2 and 3 on SJP5.
5. To connect the amplifier outputs to the ADC input, short positions 1 and 2 on both SJP1 and SJP2.
6. Components L6, C62, C29, L8, L7, C28, C61, L5 form a bandpass filter with cutoff frequencies of 105 MHz and 185 MHz, respectively. Customers will need to optimize this depending on their usage requirements.

Note that the THS4509 used on this EVM is pinout compatible with the [THS4508](#), [THS4511](#), [THS4513](#), and [THS4520](#). Users can easily interchange the amplifier on this EVM and pick the appropriate amplifier based on common-mode range, power supplies, and frequency of operation. Contact your local Texas Instruments (TI) sales representative for assistance in selection of these amplifiers.

2.2.4 ADC Clock Input

Connect a filtered, low-phase-noise clock input to J4. A 1:1 transformer, T6, converts from a single-ended clock signal to a differential clock signal. Resistor R19 serves as a 50- Ω termination.

2.2.5 ADC Digital Outputs

The DDR LVDS digital output of ADS62PXX EVM is brought to a high-density Samtec connector J8 which can be used for digital capture by a logic analyzer or capture card. Since the ADC also supports a CMOS output, provisions have been made to all for the digital output data to be routed to 40-pin IDC connectors J1 and J2. Connector J1 also supports a third output option, dual-channel multiplexed CMOS output. Users wishing to make use of the CMOS output need to make the modifications listed in the bulleted list. [Section 4](#) details connection options to TI's capture solutions, the TSW1100 and TSW1200.

- Remove resistor packs with the following reference designators: RN7, RN8, RN9, and RN10.
- Install TI's SN74AVC16244 buffer into U12 and U13.

2.2.6 Jumper Selections

The EVM features several different operational modes that can be selectable through jumpers described in [Table 1](#). The EVM also features surface-mount jumpers in cases where either the signal integrity is important or the functions are rarely used. [Table 2](#) summarizes these options.

Table 1. Jumpers

Description	Reference Designator	Default Selection	Optional Selection
THS4509 powerdown selection	JP3	2-3, THS4509 off	THS4509 on
ADS62PXX pin: Control Line 3	JP5	1-2, Logic level low, normal ADC operation	Multiple choices
ADS62PXX pin: Control Line 2	JP6	1-2, Logic level low, normal ADC operation	Multiple choices
ADS62PXX pin: Control Line 1	JP7	1-2, Logic level low, normal ADC operation	Multiple choices
SCLK control, USB or onboard voltage dividers	JP8	1-2, Onboard voltage dividers - use silkscreen for configuration	2-3, USB control
SDATA control, USB or onboard voltage dividers	JP9	1-2, Onboard voltage dividers - use silkscreen for configuration	2-3, USB control
SEN control, USB or onboard voltage dividers	JP10	1-2, Onboard voltage dividers - use silkscreen for configuration	2-3, USB control
ADS62PXX pin: Reset	JP11	1-2, Selects the parallel interface	2-3, selects the SPI interface
SCLK Parallel Mode Control	JP12	Multiple options	Multiple options
SDATA Parallel Mode Control	JP13	Multiple options	Multiple options
SEN Parallel Mode Control	JP14	Multiple options	Multiple options
ADC DVDD power supply selection	JP15	2-3, Uses onboard LDO for ADC DVDD supply	1-2, Selects banana jack P1 for ADC DVDD
ADC AVDD power supply selection	JP16	2-3, Uses onboard LDO for ADC AVDD supply	1-2, Selects banana jack P3 for ADC AVDD

Table 2. Surface-Mount Jumpers

Description	Reference Designator	Default Selection	Optional Selection
Amp output or transformer input	SJP1	2-3, ADC input from SMA input J3	1-2, ADC input from THS4509 positive output
Amp output or transformer input	SJP2	2-3, ADC input from SMA input J9	1-2, ADC input from THS4509 negative output
Amp output or transformer input	SJP3	No connection, open	2-3, THS4509 amplifier positive input
Amp output or transformer input	SJP5	1-2, ADC input from SMA input J3	2-3, THS4509 amplifier negative input

3 TI ADC SPI Control Interface

This section describes the software features accompanying the EVM kit. The TI ADC SPI control software provides full control of the SPI interface, allowing users to write to any of the ADC registers found in the data sheet. For most ADS62PXX performance evaluations, users do not need to use the TI SPI control software to get evaluation results. Users only need to use the ADC SPI control software when the desired feature is inaccessible through the ADC parallel interface mode.

3.1 Installing the ADC SPI Control Software

The ADC SPI control software can be installed on a personal computer by running the setup.exe file located on the CD. This file installs the graphical user interface (GUI) along with the USB drivers needed to communicate to the USB port that resides on the EVM. When prompted, users should allow the Windows® operating system to search for device drivers by checking "Yes, this time only", as seen in [Figure 1](#). It will find the TI ADC SPI interface drivers automatically. After the software is installed, insert the USB cable to the EVM to finish the installation. The "Found New Hardware" wizard will start, and you must acknowledge that the TI ADC SPI Interface has not passed the Windows® Logo testing as shown in [Figure 2](#). After completion, the TI ADC SPI Interface should show up in the Hardware Device Manager. [Figure 3](#) shows the SPI interface in the Hardware Manager which indicates that it is ready for use.

Note: Before plugging in the USB cable for the first time, install the TI ADC SPI software. The software installs the drivers necessary for USB communication.



Figure 1. Found New Hardware

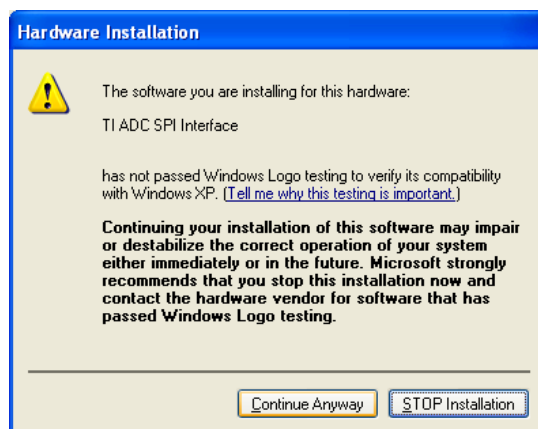


Figure 2. Window Logo Testing

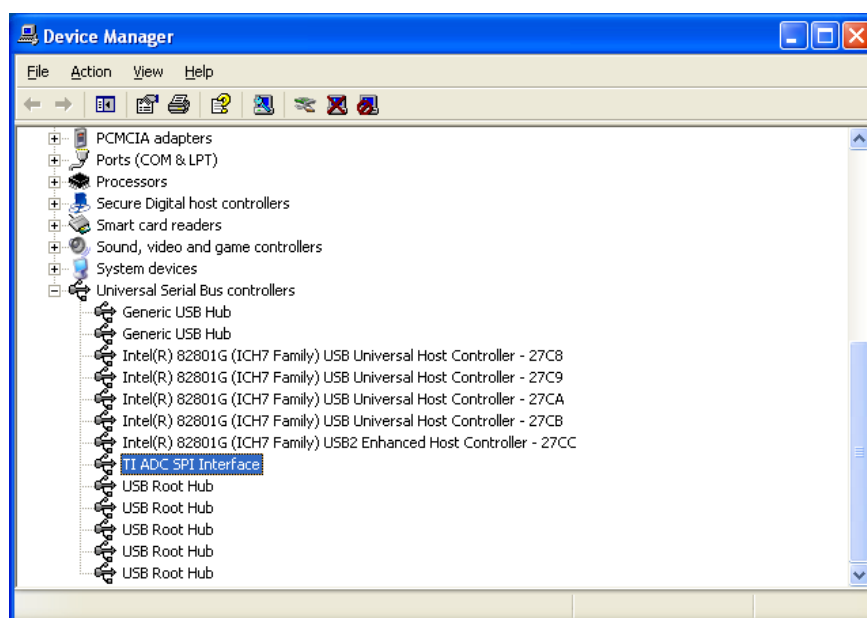


Figure 3. Hardware Device Manager

3.2 Setting Up the EVM for ADC SPI Control

Users who wish to use the ADC SPI interface must supply 5 VDC to P5, which provides power to the USB circuit. By default, the EVM comes with the ADC configured in parallel mode. In order to use the SPI interface to control the ADC modes of operation, users must move several jumpers.

- Move jumper JP11 to short positions 2–3, which places the ADC into serial operation mode.
- Move jumper JP8 to short positions 2–3, which allows the USB circuit to control SCLK.
- Move jumper JP9 to short positions 2–3, which allows the USB circuit to control SDATA.
- Move jumper JP10 to short positions 2–3, which allows the USB circuit to control SEN.

3.3 Using the TI ADC SPI Interface Software

Once the software is installed and the USB cable is connected, three primary modes of operating the software are available: SPI Register Writes, SPI Register Write Using a Script File, and ADS62PXX Frequently Used Registers.

Note: Before beginning and ADC evaluation, users are required to reset the ADC. This can easily be done by pressing the ADS62PXX Reset button found on the ADS62PXX tab. For most ADS62PXX evaluations that make use of the SPI interface, users should also assert the Over-Ride Bit also found on the ADS62PXX tab. This will force the ADC to be configured by the SPI interface only and it will ignore any board-level settings that may have been set. Please consult the datasheet for a full list of available functions in SPI interface mode.

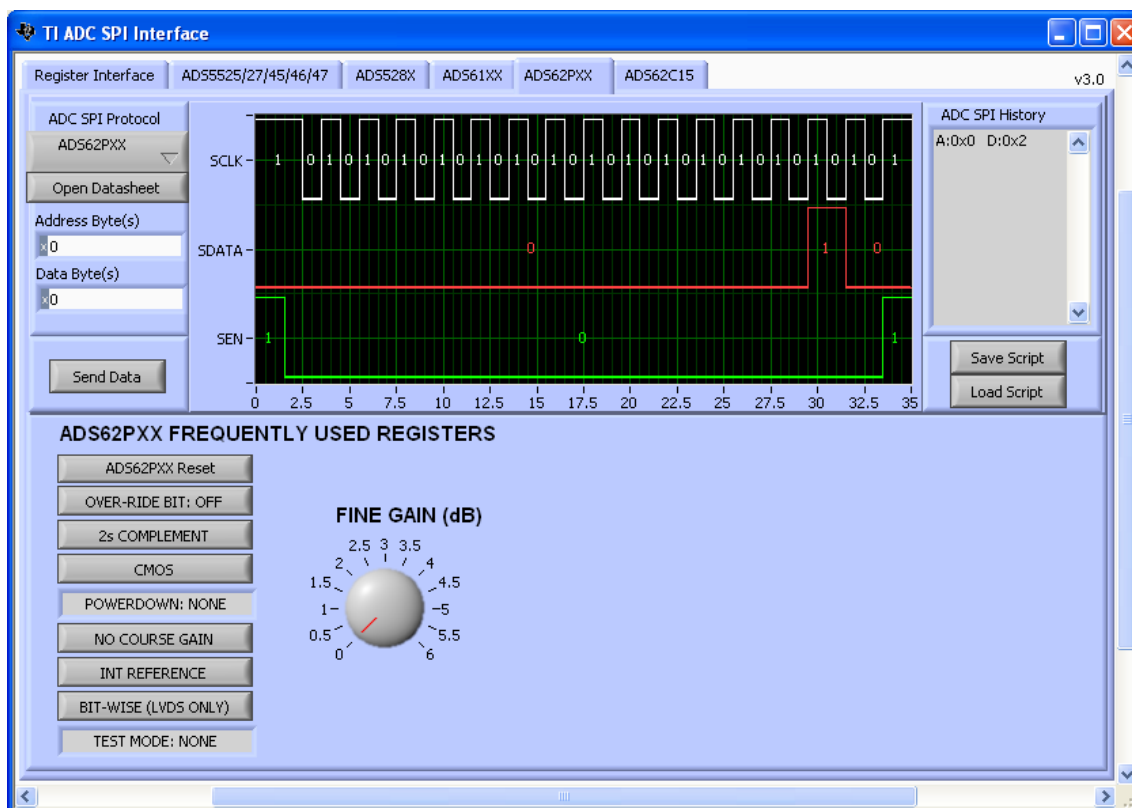


Figure 4. SPI Interface Screen

3.3.1 SPI Register Writes

The most basic mode of operation allows full control of writing to individual register addresses. In the top-left corner of the interface screen (Figure 4), select the ADS62PXX ADC from the ADC SPI Protocol drop-down list. Next, type the Address Bytes(s) in hexadecimal (hex) and Data Byte(s) in hex, which can be found in the device data sheet. When you are ready to send this command to the ADC, either press "Enter" on your keyboard or press the Send Data button. The graph indicator is updated with the patterns sent to the ADC. The default inputs to both the Address Byte(s) and Data Byte(s) fields are hex inputs as designated by the small x in the control. Users can change the default input style by clicking on the "x" to binary, decimal, octal, or hex. Multiple register writes can be written simply by changing the contents of the Address Byte(s) and Data Byte(s) field and pressing "Enter" or Send Data again. The ADC SPI History window will keep track of the register writes performed in a session.

3.3.2 SPI Register Write Using a Script File

After the ADC is configured to the desired usage, users can save time in future ADC configurations by saving a script file. By pressing the Save Script button, it dumps ADC SPI History window contents into a text file. Alternatively, users can edit the script file in a text editor. An example script file is located in the \\Install Directory\\Script Files\\ADS62P45_LVDS_oBinary.txt which configures the ADC for use with the

TSW1200. When ready to write the contents of the script file to the ADC, users can press the Load Script button and they will be prompted for the file location of their script file. The commands are sent to the ADC when the user acknowledges the selection of the file, however the graph indicator does not show multiple writes. The ADC SPI History will update show be updated to show the register writes executed in the script file.

3.3.2.1 ADS62PXX Frequently Used Registers

For ease of use, several buttons have been added that allow one-click register writes of commonly used features found in [Table 3](#). These are found in the ADS62PXX tab, as these commands are specific to the ADS62PXX ADC only. The software writes to the ADC both the contents of the associated address and data when the button is clicked. When the ADS62PXX Reset button is pressed, it issues a software reset to the ADC, and it resets the button values to match the contents inside of the ADC. The graph indicator plots the SPI commands written to the ADC when a button has been depressed.

Table 3. ADS62PXX Frequently Used Registers

Default Value	Alternate Value
ADS62PXX Reset	
Over-ride bit: Off	Over-ride bit: On
2s Complement	Straight Binary
CMOS	DDR LVDS
Powerdown: OFF	Multiple Powerdown Options
No Course Gain	3.5-dB Course Gain
INT Reference	EXT Reference
Bit-Wise (LVDS Only)	Byte-Wise
Test Mode: None	Multiple Options
Fine Gain	Multiple Options

4 Connecting to FPGA Platforms

The ADS62PXX EVM provides several connection options to use the EVM with various FPGA development platforms and FPGA-based capture boards. The ADC features two output options, a DDR LVDS which easily interfaces with a TSW1200 capture card, and a CMOS output which interfaces with a TSW1100 capture card.

4.1 TSW1200

By default, the ADS62PXX EVM natively plugs into the TSW1200 FPGA platform. The TSW1200 Rev B and Rev C can be configured for capture support, allowing ADC analysis capability. For this option, please configure the ADS62PXX to output DDR LVDS data in an offset-binary fashion. Users should consult the TSW1200 documentation for configuration details. For users wishing to control the TSW1200 over the ADS62PXX SPI interface, move the surface-mount jumpers into the following positions. It should be noted that this is not needed for most evaluations, it is merely offered as a convenience option.

- Move the jumper on JP10 (SEN) to the 1–2 position, and remove R47 and populate R70 with a 0-Ω resistor.
- Move the jumper on JP8 (SCLK) to the 1–2 position, and remove R30 while installing the 0-Ω resistor to R69.
- Move the jumper on JP9 (SDATA) to the 1–2 position, and remove R33 while installing the 0-Ω resistor to R68.
- Move the jumper on JP11 to position 2–3 to configure the ADC into the SPI operation mode (serial interface mode).

4.2 TSW1100

When the ADS62PXX is configured in CMOS output mode users can use TI's [TSW1100](#) capture board. Several additional board configuration steps are required before using this option.

- Remove resistor packs with the following reference designators: RN7, RN8, RN9, and RN10.
- Install TI's SN74AVC16244 buffer into U12 and U13.
- If using the parallel interface mode (JP11=1-2), configure the ADC in CMOS output mode using the silkscreen on JP14.

5 ADC Evaluation

This section describes how to set up a typical ADC evaluation system that is similar to what TI uses to perform testing for data-sheet generation. Consequently, the information in this section is generic in nature and is applicable to all high-speed, high-resolution ADC evaluations. This section covers signal tone analysis, which yields ADC data-sheet figures of merit such as signal-to-noise ratio (SNR) and spurious free dynamic range (SFDR).

5.1 Hardware Selection

To reveal the true performance of the ADC under evaluation, great care should be taken in selecting both the ADC signal source and ADC clocking source.

5.1.1 Analog Input Signal Generator

When choosing the quality of the ADC analog input source, consider both the harmonic distortion performance of the signal generator and the noise performance of the source.

In many cases, the harmonic distortion performance of the signal generator is inferior to that of the ADC, and additional filtering is needed if users expect to reproduce the ADC SFDR numbers found in the data sheet. Users can easily evaluate the harmonic distortion of the signal generator by hooking it directly to a spectrum analyzer, measuring the power of the output signal, and comparing that to the power of the integer multiples of the output signal frequency. If the harmonic distortion is worse than the ADC under evaluation, the ADC digitizes the performance of the signal generator and the true SFDR of the ADC is masked. To alleviate this, it is recommended that users provide additional LC filtering after the signal-generator output.

Another important metric when deciding on a signal generator is its noise performance. As with the distortion performance, if the noise performance is worse than that of the ADC under evaluation, the ADC digitizes the performance of the source. Noise can be broken into two components, broadband noise and close-in phase noise. Broadband noise can be improved by adding an LC filter to improve distortion performance; however, the close-in phase noise typically cannot be improved by additional filtering. Therefore, when selecting an analog signal source, it is important to review the manufacturer's phase noise plots and take care to choose a signal generator with the best phase-noise performance.

5.1.2 Clock Signal Generator

Equally important in the high-performance ADC evaluation setup is the selection of the clocking source. Most modern ADCs, the ADS62PXX included, accept either a sinusoidal or a square-wave clock input. The key metric in selecting a clocking source is selecting a source with the lowest jitter. This becomes increasingly important as the ADC input frequency (f_{in}) increases, because the ADC SNR evaluation setups can become jitter-limited (t_j) as shown by the following equation.

$$\text{SNR (dBc)} = 20 \log (2\pi \times f_{in} \times t_j(\text{rms}))$$

In theory, a square-wave source with femtosecond jitter would be ideal for an ADC evaluation setup. However, in practical terms, most commercially available square-wave generators offer jitter measured in picoseconds, which is too great for high-resolution ADC evaluation setups. Therefore, most evaluation setups rely on the ADC internal clock buffer to convert a sinusoidal input signal into a ultralow-jitter square wave. When selecting a sinusoidal clocking source, it has been shown that phase noise has a direct impact on jitter performance. Consequently, great scrutiny should be applied to the phase-noise performance of the clocking signal generator. TI has found that high-Q monolithic crystal filters can improve the phase noise of the signal generator, and these filters become essential elements of the evaluation setup when high ADC input frequencies are being evaluated.

5.2 Coherent Input Frequency Selection

Typical ADC analysis requires users to collect the resulting time-domain data and perform a Fourier transform to analyze the data in the frequency domain. A stipulation of the Fourier transform is that the signal must be continuous-time; however, this is impractical when looking at a finite set of ADC samples, usually collected from a logic analyzer. Consequently, users typically apply a window function to minimize the time-domain discontinuities that arise when analyzing a finite set of samples. For ADC analysis, window functions have their own frequency signatures or lobes that distort both SNR and SFDR measurements of the ADC.

TI uses the concept of coherent sampling to work around the use of a window function. The central premise of coherent sampling entails that the input signal into the ADC is carefully chosen such that when a continuous-time signal is reconstructed from a finite sample set, no time-domain discontinuities exist. To achieve this, the input frequency must be an integer multiple of the ratio of the ADC sample rate (f_s) and the number of samples collected from the logic analyzer (N_s). The ratio of f_s to N_s is typically referred to as the fundamental frequency (f_f). Determining the ADC input frequency is a two-step process. First, the users select the frequency of interest for evaluating the ADC; then, they divide this by the fundamental frequency. This typically yields a non-integer value, which should be rounded to the nearest odd, preferably prime, integer. Once that integer, or frequency bin (f_{bin}), has been determined, users multiply this with the fundamental frequency to obtain a coherent frequency to program into their ADC input signal generator. The procedure is summarized as follows.

$$f_f = f_s / N_s$$

$$f_{bin} = \text{Odd_round}(f_{desired} / f_f)$$

$$\text{Coherent frequency} = f_f \times f_{bin}$$

6 Physical Description

This section describes the physical characteristics and PCB layout of the EVM.

6.1 PCB Layout

The EVM is constructed on a four-layer, 0.062-inch thick PCB using FR-4 material. The individual layers are shown in [Figure 5](#) through [Figure 8](#). The layout features a split ground plane; however, similar performance can be obtained with careful layout using a common ground plane.

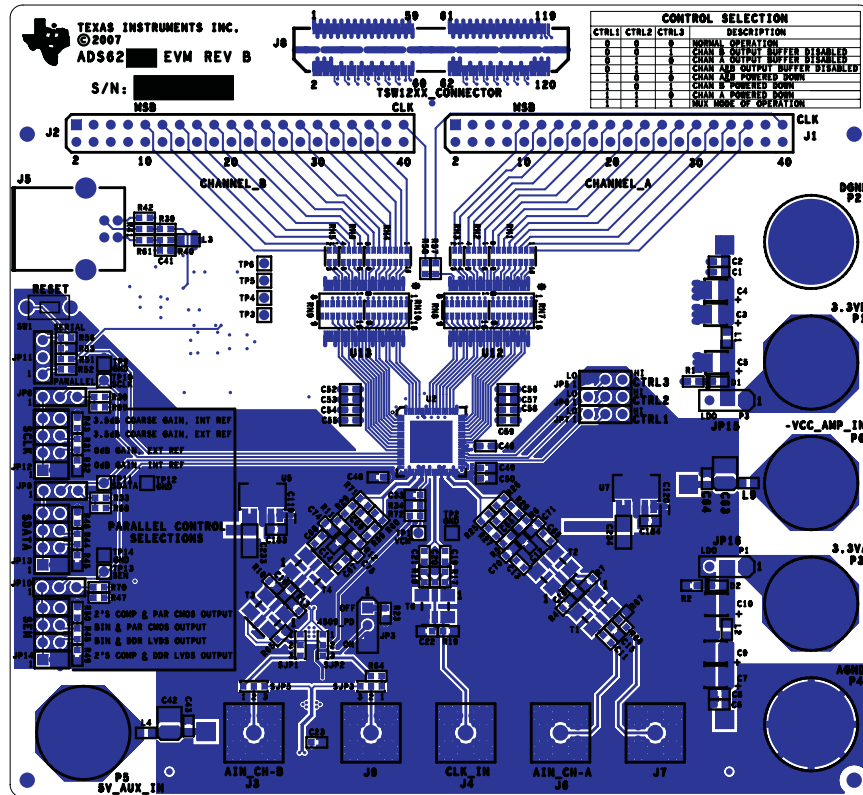


Figure 5. Top Silkscreen

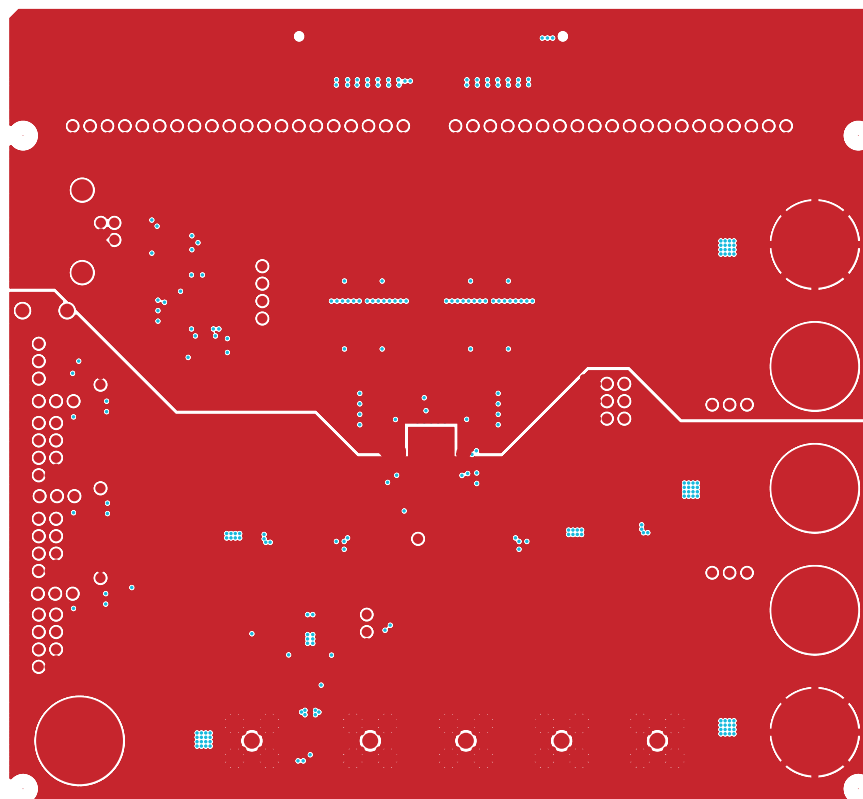


Figure 6. Component Side

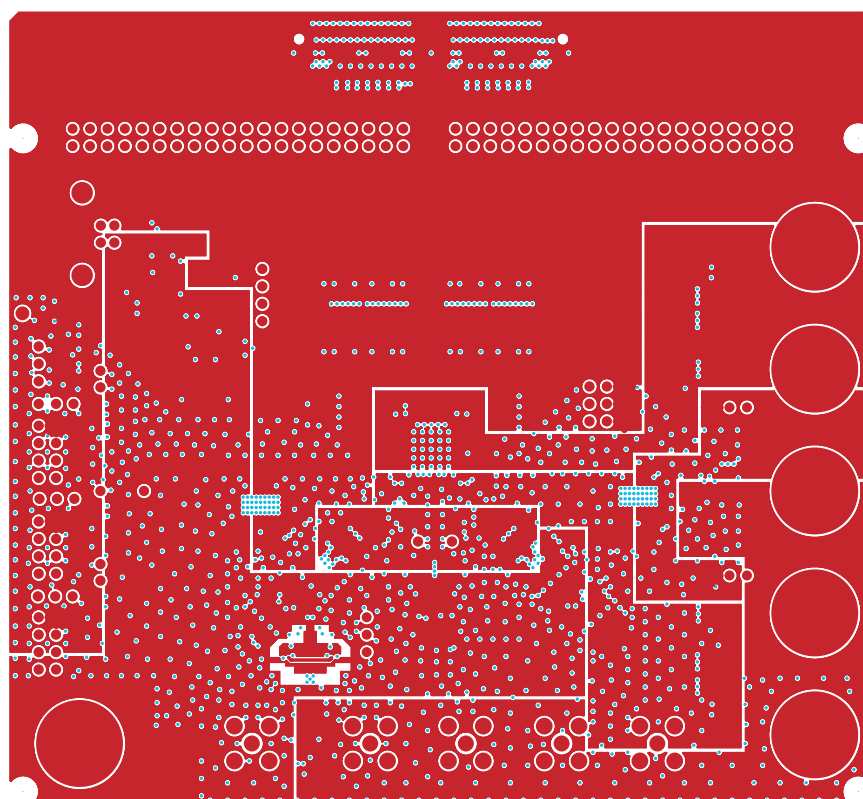


Figure 7. Power Plane 1

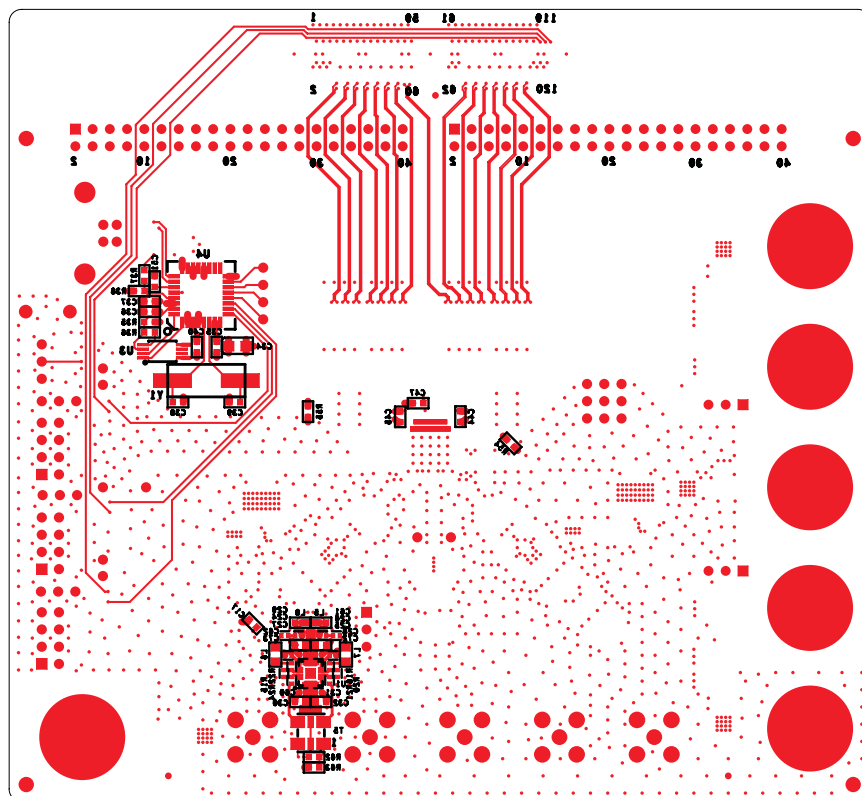


Figure 8. Bottom Side

6.2 Bill of Materials

Table 4. Bill of Materials

Qty	Reference	Value	Footprint	MFR	Part Number	DNI = Do Not Install
4	C1,C6,C43,C64	1μF	603	Panasonic	ECJ-1VB1A105K	
15	C2, C8, C19–C23, C52–C59	0.1μF	603	Panasonic	ECJ-1VB1C104K	
4	C3, C5, C7, C10	22μF	smd_cap_1210_pol	Kemet	T491A226M010AT	
2	C4, C9	10μF	smd_cap_1210_pol	Kemet	B45197A3106K209	
23	C11–C18, C33,C35–C37, C40,C44–C50, C66–C68	0.1μF	603	Murata	GRM188R71H104KA93D	
4	C24, C26, C30, C32	10μF	603	Murata	GRM188R60J106ME47D	
6	C25, C27, C31, C60, C72,C73	0.1μF	402	Panasonic	ECJ-0EB1C104K	
2	C28, C62	4.7pF	402	Panasonic	ECD-G0E4R7C	
2	C29, C61	5pF	402	Panasonic	ECJ-0EC1H050C	
1	C34	10μF	TANT_A	Kemet	T491A106M006AS	
2	C38, C39	27pF	603	Murata	GRM1885C2A270JA01D	
1	C41	0.01μF	603	Kemet	C0603C103K1RACTU	
2	C42, C63	33μF	TANT_B	Kemet	B45196H1336K209	
1	C51	33nF	603	AVX	06035C333KAT2A	
0	C65, C69	3.3pF	603	Panasonic	ECJ-1VC1H3R30C_DNI	DNI
4	C70, C71, C74, C75	5.6pF	603	AVX	06035A5R6CAT2A_DNI	DNI
2	C119, C120	0.01μF	402	Panasonic	ECJ-0EB1E103K	
2	C183, C184	1μF	603	Panasonic	ECJ-1V41E105M	
2	C233, C234	2.2μF	1206	Panasonic	ECJ-HVB1A225K	
2	D1, D2	GREEN	603	Panasonic	LNJ312G8TRA	
3	JP3, JP15, JP16	HEADER_1x3_100_430L		Samtec	HMTSW-103-07-G-S-.240	(SHUNT 2-3)
7	JP5–JP11	HEADER_1x3_100_430L		Samtec	HMTSW-103-07-G-S-.240	(SHUNT 1-2)
1	JP13	HEADER 4x2		Molex	90131-0124	
2	JP12, JP14	HEADER 4x2		Molex	90131-0124	(SHUNT 1-2)
2	J1, J2	HMTSW-120-07-G-D-.240		Samtec	HMTSW-120-07-G-D-.240	
4	J3, J4, J6, J9	SMA		Johnson Components	142-0701-201	
1	J5	CONN USB TYP B FEM		Milmax	897-43-004-90-000	
0	J7	SMA		Johnson Components	142-0701-201	DNI
1	J8	CONN_QTH_30X2-D-A		Samtec	QTH-060-02-F-D-A	
2	L1,L2	68 at 100MHz	603	Steward	MI0603J680R-10	
1	L3	1K at 100MHZ	805	Murata	BLM21AG102SN1D	
2	L4,L9	68 at 100MHz	603	Steward	MI0603J680R-10	
2	L5,L8	47nH	603	Coilcraft	0603CS-47NXJL	
2	L6,L7	150	805	API Delavan Inc	0805-151J	
1	P1	3.3VD		Allied Electronics	ST-351A	
1	P2	DGND		Allied Electronics	ST-351B	
1	P3	3.3VA		Allied Electronics	ST-351A	
1	P4	AGND		Allied Electronics	ST-351B	
1	P5	5V_AUX_IN		Allied Electronics	ST-351A	
1	P6			Allied Electronics	ST-351A	
2	RN1,RN4	22	met8_16_0603	CTS	742C163220JTR	
2	RN2,RN6	22	met4_8_0603	Panasonic	EXB-38V220JV	
2	RN3,RN5	22	met2_4_0603	Panasonic	EXB-34V220JV	
4	RN7–RN10	0 Ω	met8_16_0603	CTS	742C163000X	
2	R1,R2	750	603	Panasonic	ERJ-3EKF7500V	
8	R4–R7, R10–R13	49.9	603	Panasonic	ERJ-3EKF49R9V	
2	R15, R20	348	402	Panasonic	ERJ-2RKF3480X	
2	R16, R22	68	402	Yageo Corporation	RC0402FR-0768RL	
0	R17, R18	121	603	Panasonic	ERJ-3EKF1210V	DNI
1	R19	49.9	603	Panasonic	ERJ-3EKF49R9V	
2	R21, R24	100	402	Panasonic	ERJ-2RKF1000X	
1	R23	10K	603	Panasonic	ERJ-3EKF1002V	

Table 4. Bill of Materials (continued)

Qty	Reference	Value	Footprint	MFR	Part Number	DNI = Do Not Install
0	R25, R26, R60, R71	49.9	603	Panasonic	ERJ-3EKF49R9V_DNI	DNI
4	R27, R28, R29, R59	4.99	603	Yageo	RC0603FR-074R99L	
8	R30, R33, R34, R47, R54, R55, R61, R72	0 Ω	603	Panasonic	ERJ-3GEY0R00V	
9	R31, R32, R43–R46, R48–R50	1K	603	Panasonic	ERJ-3EKF1001V	
1	R35	10K	603	Panasonic	ERJ-3GEYJ103V	
1	R36	2.21K	603	Panasonic	ERJ-3EKF2211V	
1	R37	4.7K	603	Panasonic	ERJ-3GEYJ472V	
0	R38	10K	603	Panasonic	ERJ-3EKF1002V_DNI	DNI
1	R39	1.5K	603	Panasonic	ERJ-3EKF1501V	
0	R40, R68–R70	0 Ω	603	Panasonic	ERJ-3GEY0R00V_DNI	DNI
2	R41, R42	26.7	603	Panasonic	ERJ-3EKF26R7V	
2	R51, R56	10	603	Panasonic	ERJ-3EKF10R0V	
2	R52, R53	10K	603	Panasonic	ERJ-3EKF1002V	
2	R57, R58	22	603	Yageo	RC0603FR-0722RL	
0	R62, R64, R66	0 Ω	603	DALE	CRCW06030000Z0EA_DNI	DNI
3	R63, R65, R67	0 ohm	603	DALE	CRCW06030000Z0EA	
0	SJP1, SJP2	JUMPER_1x3_SMT	SMD_BRIDGE_1x3_0603	DNI	DNI	(SHUNT 2-3)
0	SJP3	JUMPER_1x3_SMT	SMD_BRIDGE_1x3_0603	DNI	DNI	(NO SHUNT)
0	SJP5	JUMPER_1x3_SMT	SMD_BRIDGE_1x3_0603	DNI	DNI	(SHUNT 1-2)
1	SW1	SW PUSHBUTTON	SW_RESET_PTS635	C & K Switch	PTS635SL43	
4	TP1, TP10, TP11, TP13	Test Point White	testpoint	Keystone	5002	
4	TP2, TP9, TP12, TP14	Test Point Black	testpoint	Keystone	5001	
4	TP3–TP6	T POINT R	TESTPOINT	Keystone	5002	
5	T1–T5	WBC1-1TL	XFMR_TC4-1W	Coilcraft	WBC1-1TL	
1	T6	TC1-1T	XFMR_TC4-1W	Minicircuits	TC1-1T	
1	U1	THS4509	QFN16	Texas Instruments	THS4509RGTT	
1	U2	ADS62PXX	QFN64	Texas Instruments	ADS62PXX	
1	U3	93C66B	TSSOP8	Microchip	93C66B	
1	U4	FT245BM	PQFP32	Future Technology Devices	FT245BM	
2	U5, U7	TPS79633DCQ	SOT_223_6_TG	Texas Instruments	TPS79633DCQ	
0	U12, U13	SN74AVC16244DGGR	TSSOP_48_496x244_20	Texas Instruments	SN74AVC16244DGGR_DNI	DNI
1	Y1	6.0000MHz	smd_csm-7_xtal	ECS	ECS-60-32-5PDN-TR	
10	Z_SH-H1	SHUNT-HEADER		Keltron	MJ-5.97-G or equivalent	SHUNT FOR HEADER
3	Z_SH-J1, Z_SH-J2, Z_SH-J5	SHUNT-JUMPER-0603		Panasonic	ERJ-3GE0R00X	SHUNT FOR JUMPER
4	Z_STANDOFF SCREW1, Z_STANDOFF SCREW2, Z_STANDOFF SCREW3, Z_STANDOFF SCREW4	PANHEAD SCREW 4-40 x 3/8		Building Fasteners	PMS 440 0038 PH	SCREW FOR STANDOFF
4	Z_STANDOFF1, Z_STANDOFF2, Z_STANDOFF3, Z_STANDOFF4	STANDOFF ALUM HEX 4-40 x .500		Keystone	2203	STANDOFF

6.3 EVM Schematics

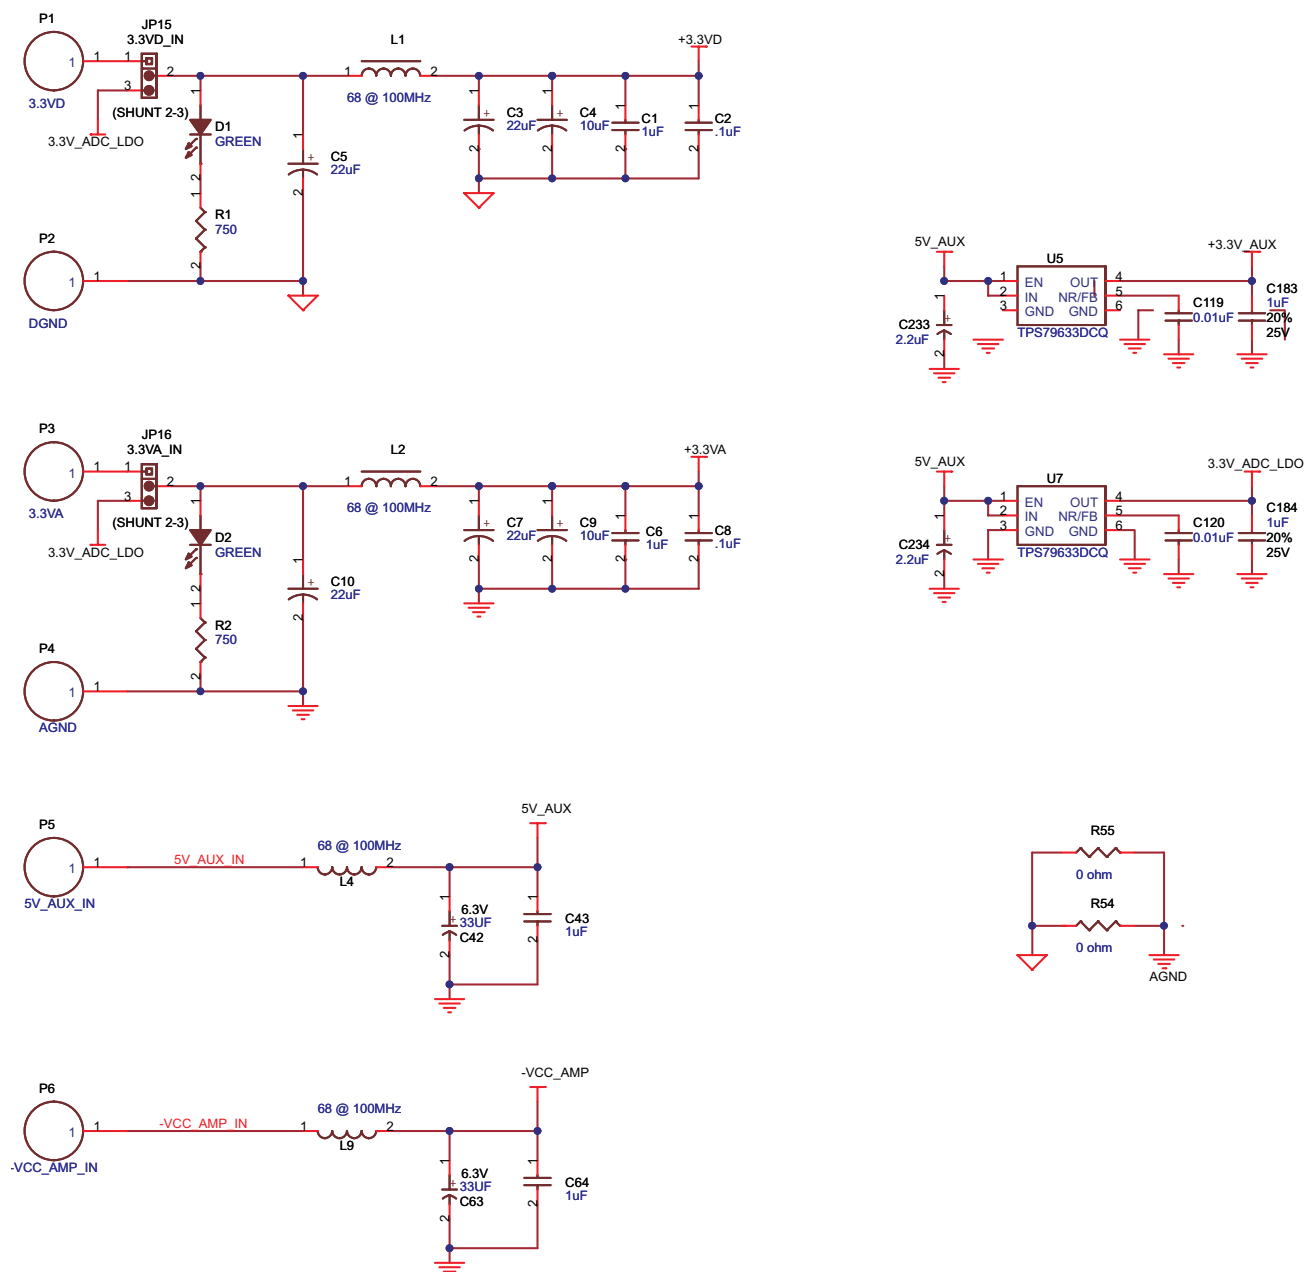


Figure 9. EVM Schematic, Sheet 1

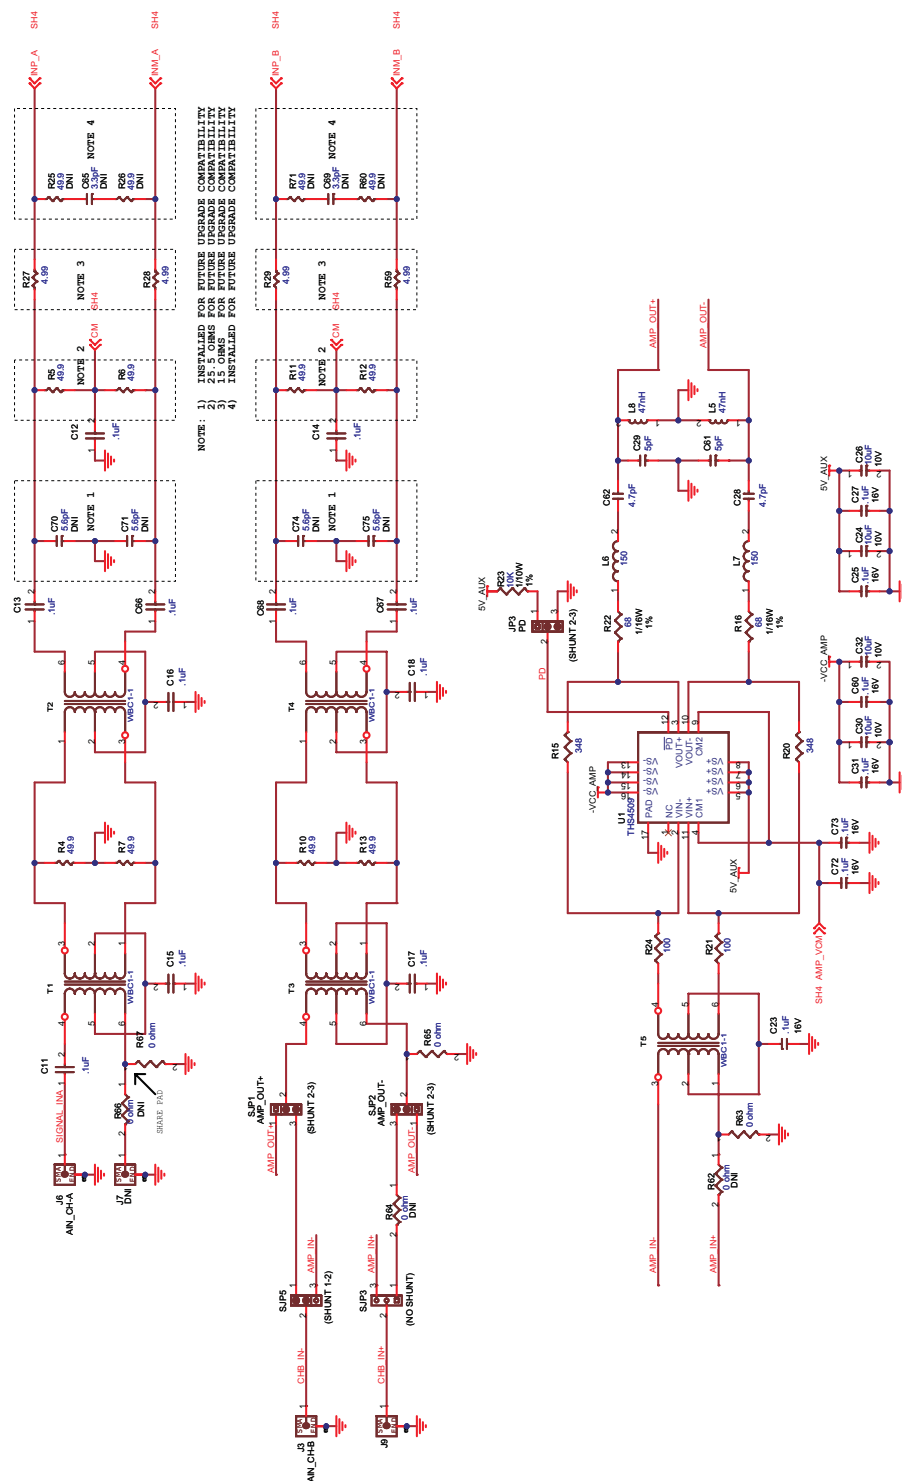


Figure 10. EVM Schematic, Sheet 2

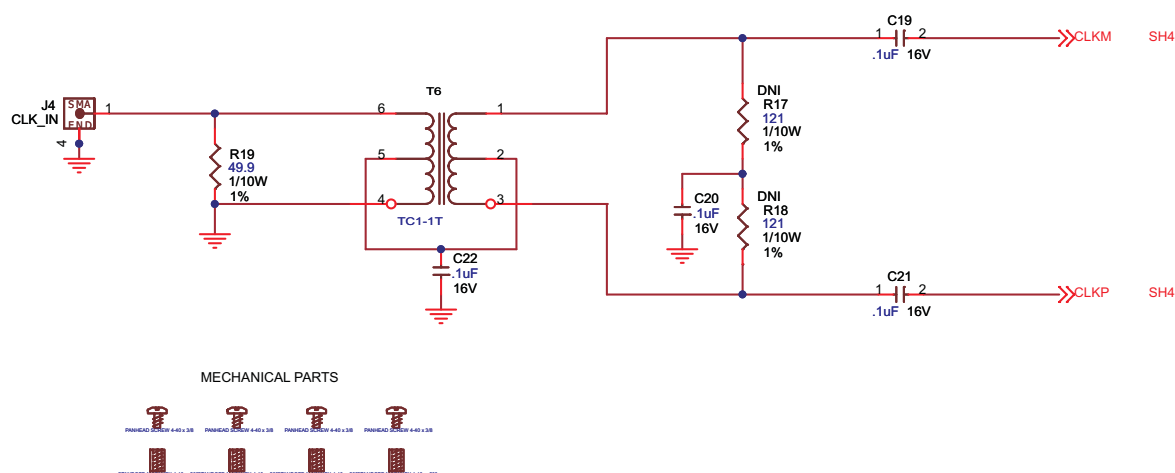


Figure 11. EVM Schematic, Sheet 3

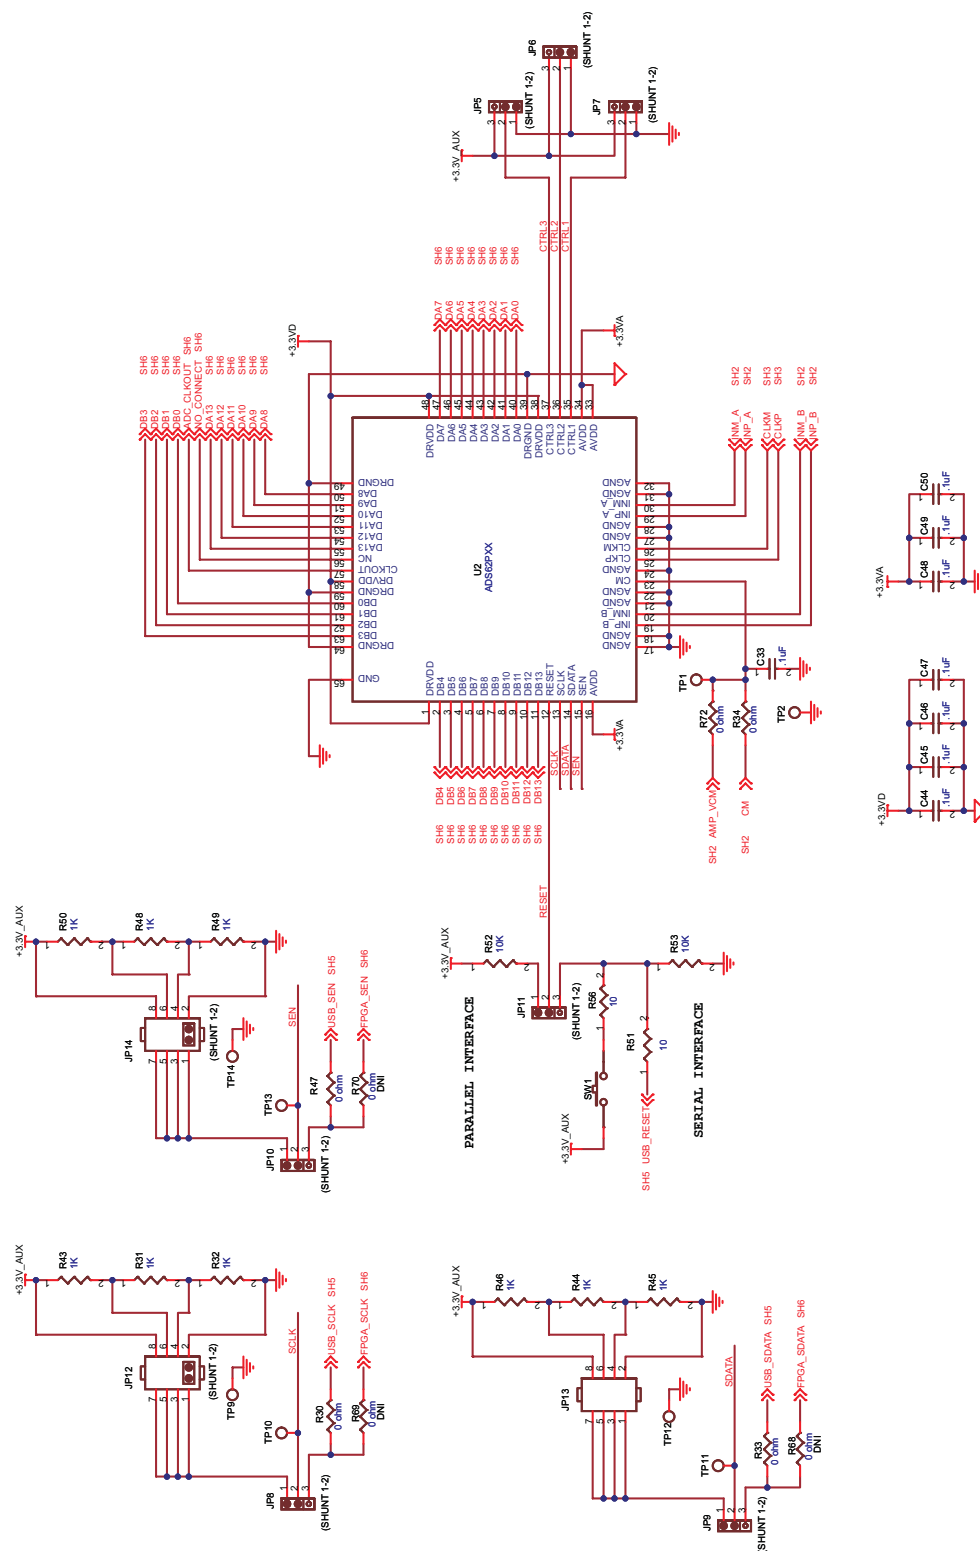


Figure 12. EVM Schematic, Sheet 4

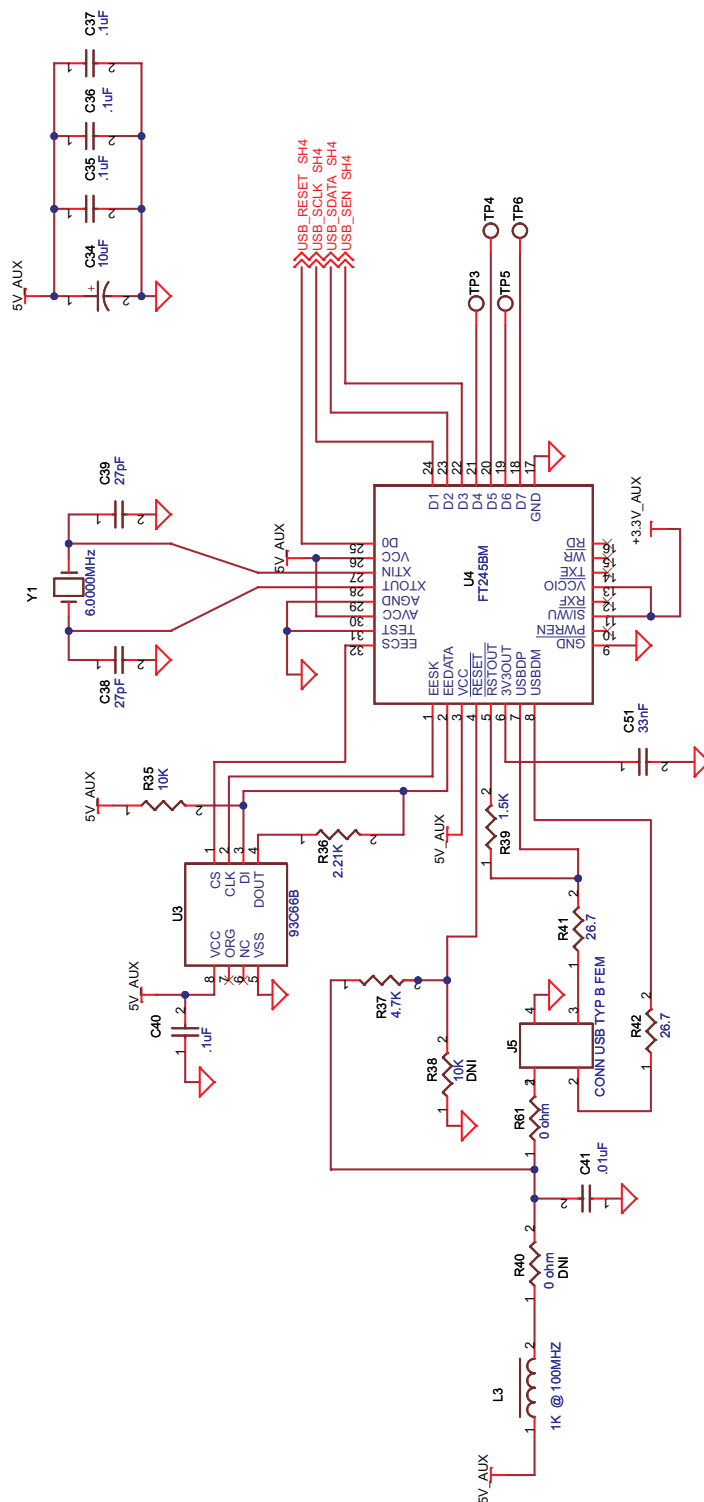


Figure 13. EVM Schematic, Sheet 5

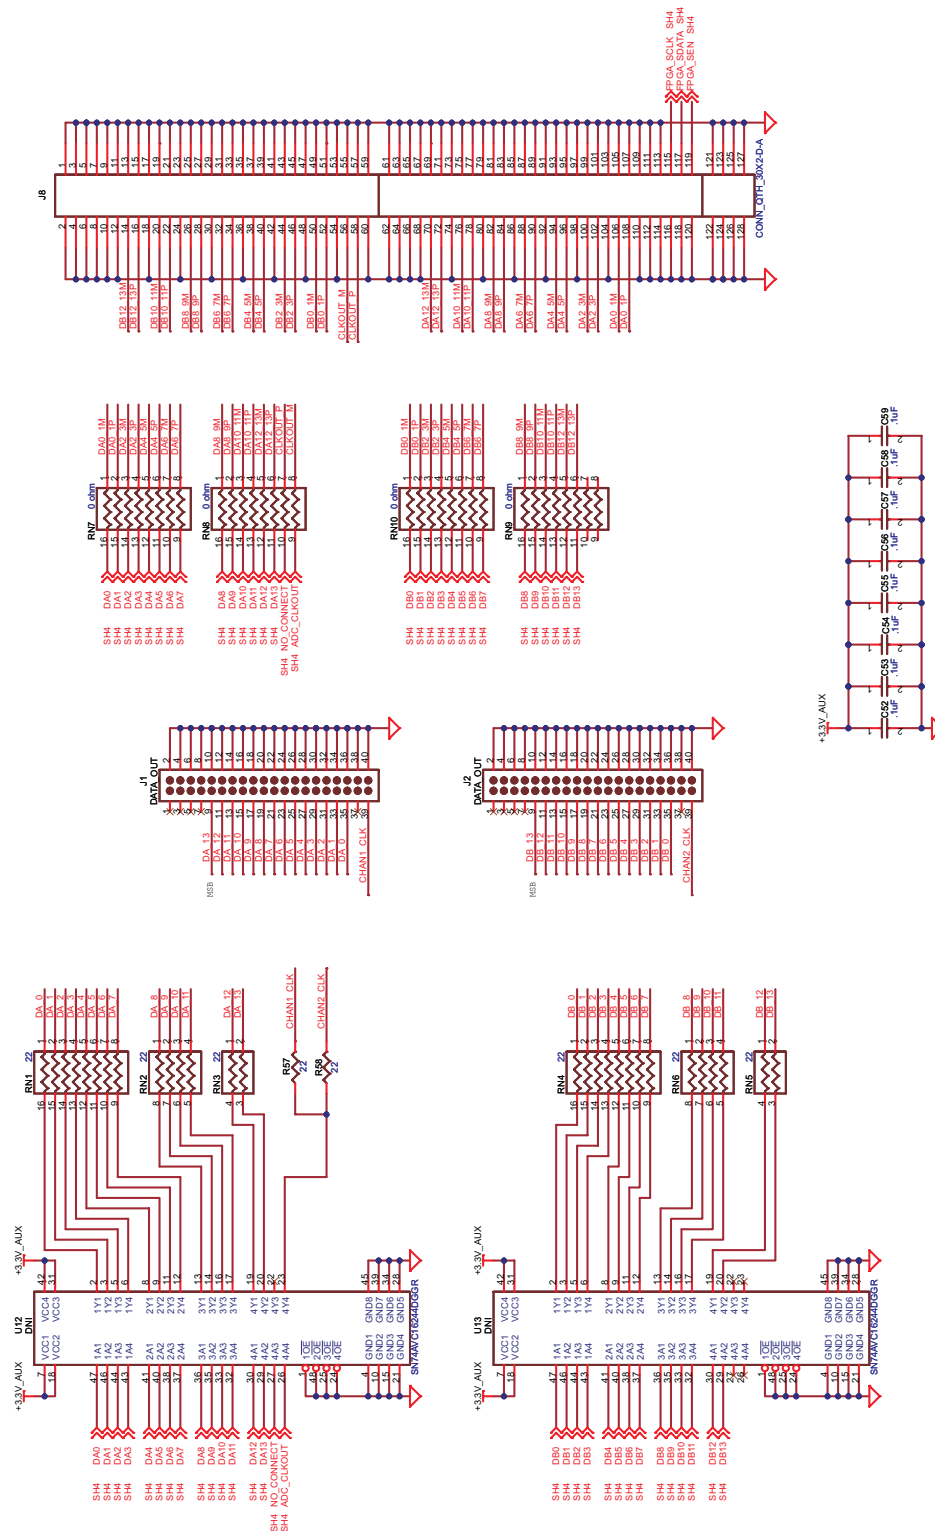


Figure 14. Breakout Board Schematic, Sheet 6

EVALUATION BOARD/KIT IMPORTANT NOTICE

Texas Instruments (TI) provides the enclosed product(s) under the following conditions:

This evaluation board/kit is intended for use for **ENGINEERING DEVELOPMENT, DEMONSTRATION, OR EVALUATION PURPOSES ONLY** and is not considered by TI to be a finished end-product fit for general consumer use. Persons handling the product(s) must have electronics training and observe good engineering practice standards. As such, the goods being provided are not intended to be complete in terms of required design-, marketing-, and/or manufacturing-related protective considerations, including product safety and environmental measures typically found in end products that incorporate such semiconductor components or circuit boards. This evaluation board/kit does not fall within the scope of the European Union directives regarding electromagnetic compatibility, restricted substances (RoHS), recycling (WEEE), FCC, CE or UL, and therefore may not meet the technical requirements of these directives or other related directives.

Should this evaluation board/kit not meet the specifications indicated in the User's Guide, the board/kit may be returned within 30 days from the date of delivery for a full refund. **THE FOREGOING WARRANTY IS THE EXCLUSIVE WARRANTY MADE BY SELLER TO BUYER AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED, IMPLIED, OR STATUTORY, INCLUDING ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR ANY PARTICULAR PURPOSE.**

The user assumes all responsibility and liability for proper and safe handling of the goods. Further, the user indemnifies TI from all claims arising from the handling or use of the goods. Due to the open construction of the product, it is the user's responsibility to take any and all appropriate precautions with regard to electrostatic discharge.

EXCEPT TO THE EXTENT OF THE INDEMNITY SET FORTH ABOVE, NEITHER PARTY SHALL BE LIABLE TO THE OTHER FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES.

TI currently deals with a variety of customers for products, and therefore our arrangement with the user **is not exclusive**.

TI assumes **no liability for applications assistance, customer product design, software performance, or infringement of patents or services described herein.**

Please read the User's Guide and, specifically, the Warnings and Restrictions notice in the User's Guide prior to handling the product. This notice contains important safety information about temperatures and voltages. For additional information on TI's environmental and/or safety programs, please contact the TI application engineer or visit www.ti.com/esh.

No license is granted under any patent right or other intellectual property right of TI covering or relating to any machine, process, or combination in which such TI products or services might be or are used.

FCC Warning

This evaluation board/kit is intended for use for **ENGINEERING DEVELOPMENT, DEMONSTRATION, OR EVALUATION PURPOSES ONLY** and is not considered by TI to be a finished end-product fit for general consumer use. It generates, uses, and can radiate radio frequency energy and has not been tested for compliance with the limits of computing devices pursuant to part 15 of FCC rules, which are designed to provide reasonable protection against radio frequency interference. Operation of this equipment in other environments may cause interference with radio communications, in which case the user at his own expense will be required to take whatever measures may be required to correct this interference.

EVM WARNINGS AND RESTRICTIONS

It is important to operate this EVM within the input voltage range of -0.3 V to 5.6 V and the output voltage range of -0.3 V to 5.6 V .

Exceeding the specified input range may cause unexpected operation and/or irreversible damage to the EVM. If there are questions concerning the input range, please contact a TI field representative prior to connecting the input power.

Applying loads outside of the specified output range may result in unintended operation and/or possible permanent damage to the EVM. Please consult the EVM User's Guide prior to connecting any load to the EVM output. If there is uncertainty as to the load specification, please contact a TI field representative.

During normal operation, some circuit components may have case temperatures greater than 50°C . The EVM is designed to operate properly with certain components above 25°C as long as the input and output ranges are maintained. These components include but are not limited to linear regulators, switching transistors, pass transistors, and current sense resistors. These types of devices can be identified using the EVM schematic located in the EVM User's Guide. When placing measurement probes near these devices during operation, please be aware that these devices may be very warm to the touch.

Mailing Address: Texas Instruments, Post Office Box 655303, Dallas, Texas 75265
Copyright = 2007-2008, Texas Instruments Incorporated

IMPORTANT NOTICE

Texas Instruments Incorporated and its subsidiaries (TI) reserve the right to make corrections, modifications, enhancements, improvements, and other changes to its products and services at any time and to discontinue any product or service without notice. Customers should obtain the latest relevant information before placing orders and should verify that such information is current and complete. All products are sold subject to TI's terms and conditions of sale supplied at the time of order acknowledgment.

TI warrants performance of its hardware products to the specifications applicable at the time of sale in accordance with TI's standard warranty. Testing and other quality control techniques are used to the extent TI deems necessary to support this warranty. Except where mandated by government requirements, testing of all parameters of each product is not necessarily performed.

TI assumes no liability for applications assistance or customer product design. Customers are responsible for their products and applications using TI components. To minimize the risks associated with customer products and applications, customers should provide adequate design and operating safeguards.

TI does not warrant or represent that any license, either express or implied, is granted under any TI patent right, copyright, mask work right, or other TI intellectual property right relating to any combination, machine, or process in which TI products or services are used. Information published by TI regarding third-party products or services does not constitute a license from TI to use such products or services or a warranty or endorsement thereof. Use of such information may require a license from a third party under the patents or other intellectual property of the third party, or a license from TI under the patents or other intellectual property of TI.

Reproduction of TI information in TI data books or data sheets is permissible only if reproduction is without alteration and is accompanied by all associated warranties, conditions, limitations, and notices. Reproduction of this information with alteration is an unfair and deceptive business practice. TI is not responsible or liable for such altered documentation. Information of third parties may be subject to additional restrictions.

Resale of TI products or services with statements different from or beyond the parameters stated by TI for that product or service voids all express and any implied warranties for the associated TI product or service and is an unfair and deceptive business practice. TI is not responsible or liable for any such statements.

TI products are not authorized for use in safety-critical applications (such as life support) where a failure of the TI product would reasonably be expected to cause severe personal injury or death, unless officers of the parties have executed an agreement specifically governing such use. Buyers represent that they have all necessary expertise in the safety and regulatory ramifications of their applications, and acknowledge and agree that they are solely responsible for all legal, regulatory and safety-related requirements concerning their products and any use of TI products in such safety-critical applications, notwithstanding any applications-related information or support that may be provided by TI. Further, Buyers must fully indemnify TI and its representatives against any damages arising out of the use of TI products in such safety-critical applications.

TI products are neither designed nor intended for use in military/aerospace applications or environments unless the TI products are specifically designated by TI as military-grade or "enhanced plastic." Only products designated by TI as military-grade meet military specifications. Buyers acknowledge and agree that any such use of TI products which TI has not designated as military-grade is solely at the Buyer's risk, and that they are solely responsible for compliance with all legal and regulatory requirements in connection with such use.

TI products are neither designed nor intended for use in automotive applications or environments unless the specific TI products are designated by TI as compliant with ISO/TS 16949 requirements. Buyers acknowledge and agree that, if they use any non-designated products in automotive applications, TI will not be responsible for any failure to meet such requirements.

Following are URLs where you can obtain information on other Texas Instruments products and application solutions:

Products

Amplifiers	amplifier.ti.com
Data Converters	dataconverter.ti.com
DSP	dsp.ti.com
Clocks and Timers	www.ti.com/clocks
Interface	interface.ti.com
Logic	logic.ti.com
Power Mgmt	power.ti.com
Microcontrollers	microcontroller.ti.com
RFID	www.ti-rfid.com
RF/IF and ZigBee® Solutions	www.ti.com/lprf

Applications

Audio	www.ti.com/audio
Automotive	www.ti.com/automotive
Broadband	www.ti.com/broadband
Digital Control	www.ti.com/digitalcontrol
Medical	www.ti.com/medical
Military	www.ti.com/military
Optical Networking	www.ti.com/opticalnetwork
Security	www.ti.com/security
Telephony	www.ti.com/telephony
Video & Imaging	www.ti.com/video
Wireless	www.ti.com/wireless

Mailing Address: Texas Instruments, Post Office Box 655303, Dallas, Texas 75265
Copyright © 2008, Texas Instruments Incorporated